

Improving Natural Gas Liquids Plant Performance with Process Gas Chromatographs

Process gas chromatographs have been used since the 1950s to provide real-time compositional data to process control systems. Today, there are tens of thousands of process gas chromatographs in use throughout the process industry making the gas chromatograph the analytical workhorse for online compositional measurements. One example of how process gas chromatographs are used for improving process operations can be found in natural gas liquids plants.

The liquids extracted from natural gas are an important source of feedstock for a number of other petrochemical processes. The ethane and propane are used as feed to ethylene plants and a refinery's alkylation unit uses the iso-butane. To separate these compounds from the natural gas liquids (NGL), a series of distillation towers is used to separate the methane and heavier streams into individual pure product streams.

The Natural Gas Liquids (NGL) Plant

Since the various hydrocarbons in the NGL stream are easily separated by their boiling point, the NGL feed moves from one distillation (fractionator) tower to another. Each tower separates one of the hydrocarbon products and sends the remaining product on to the next tower (see Figure 1).

The product moves from the demethanizer tower where the methane is removed as the overhead product stream to the deethanizer tower for the ethane and on to the depropanizer tower for the propane.

Since there are two types of butanes in the NGL stream, it takes two towers to separate them into pure product streams. The first step is the debutanizer that separates the total butanes (iso-C4 and the normal-C4) from the remaining NGL stream. The iC_4 and nC_4 are then separated from each other in the C4 splitter tower.

The C5 and heavier components remaining in the NGL stream is typically left as a C5+ product stream to be used in other processes such as refinery gasoline blending.

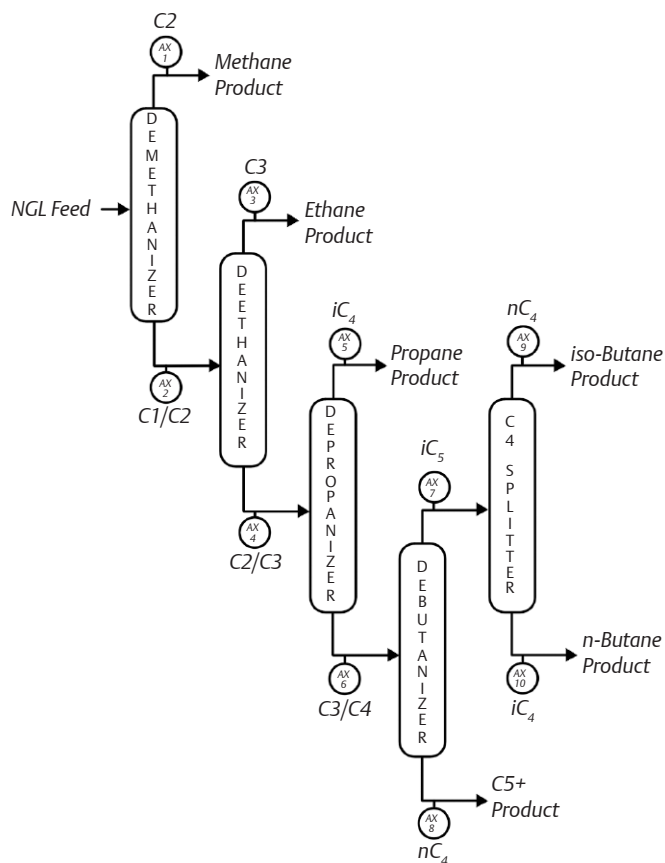


Figure 1 - Flow Diagram of a Typical NGL Plant

Improving Unit Performance with Process Gas Chromatographs

An NGL plant uses a number of process gas chromatographs since they play such a critical role in optimizing the distillation tower operation as well as assuring that each of the product streams meet specifications. This is the primary role of the analyzers AX #1, #3, #5, #8, #9 and #10 as listed on Figure 1.

On the various bottom streams, it is necessary to perform a ratio analysis. For example, on the deethanizer tower, a process gas chromatograph typically monitors the ethane product for impurities such as C3 to insure that the heavy impurities are kept within specification. However, measuring the lighter compounds like C1 is pointless at this stage because it is lighter than the product being made and can't be kept out of the overhead stream, no matter where the reflux ratio is set. To control the lighter compounds in the overheads, they must be controlled upstream before entering the tower. A ratio of the C1 to C2 on the bottom streams of the demethanizer is performed to compensate for the compositional changes that occur in the deethanizer tower (AX #2 in Figure 1).

This same ratio measurement is then done on the deethanizer bottom streams (AX #4 in Figure 1) and depropanizer bottom streams (AX #6 in Figure 1). A summary of these applications can be seen in Figure 2.

The Emerson Solution

Emerson has a long history of providing process gas chromatographs for the natural gas industry. Emerson's process gas chromatographs set the standard for online process measurement by supplying analyzers that are both robust and capable of handling the analytical requirements.

Table 1 - Summary of Process Gas Chromatograph Applications in a Typical NGL Plant

Analyzer #	Stream	Components Measured	Measurement Objective
1	Demethanizer overhead	C2	Minimize C2+ impurities in methane product
2	Demethanizer bottoms	C1, C2	Minimize C1 impurities in ethane product
3	Deethanizer overhead	C3	Minimize C3+ impurities in ethane product
4	Deethanizer bottoms	C2, C3	Minimize C2 impurities in propane product
5	Depropanizer overhead	iC ₄	Minimize iC ₄ ⁺ impurities in propane product
6	Depropanizer bottoms	C3, iC ₄	Minimize C3 impurities in iso-butane product
7	Debutanizer overhead	iC ₅	Minimize iC ₅ ⁺ impurities in n-butane product
8	Debutanizer bottoms	nC ₄	Minimize nC ₄ ⁺ impurities in C ₅ ⁺ product
9	C4 splitter overhead	nC ₄	Minimize nC ₄ ⁺ impurities in iso-butane product
10	C4 splitter bottoms	iC ₄	Minimize iC ₄ impurities in n-butane product

www.RosemountAnalytical.com



www.analyticexpert.com



www.youtube.com/user/RosemountAnalytical



www.twitter.com/RAIhome



www.facebook.com/EmersonRosemountAnalytical

©2013 Emerson Process Management. All rights reserved.

Emerson Process Management

Rosemount Analytical
Analytical Center of Excellence
10241 West Little York, Suite 200
Houston, TX 77040 USA
Toll Free 866 422 3683
T +1 713 396 8880 (North America)
T +1 713 396 8759 (Latin America)
F +1 713 466 8175
gc.csc@emerson.com

The Emerson logo is a trademark and service mark of Emerson Electric Co. Rosemount Analytical is a mark of one of the Emerson Process Management family of companies. All other marks are the property of their respective owners.

The contents of this publication are presented for information purposes only, and while effort has been made to ensure their accuracy, they are not to be construed as warranties or guarantees, express or implied, regarding the products or services described herein or their use or applicability. All sales are governed by our terms and conditions, which are available on request. We reserve the right to modify or improve the designs or specifications of our products at any time without notice.